


- Ammonia (NH₃ + NH₄⁺; as N), FIL, DA -
Blind Blank Results
Lab: NWQL, PCode: 00608, MCode: SHC02
 Analysis dates: 10/04/19 through 09/29/23
[Open Data Set](#)

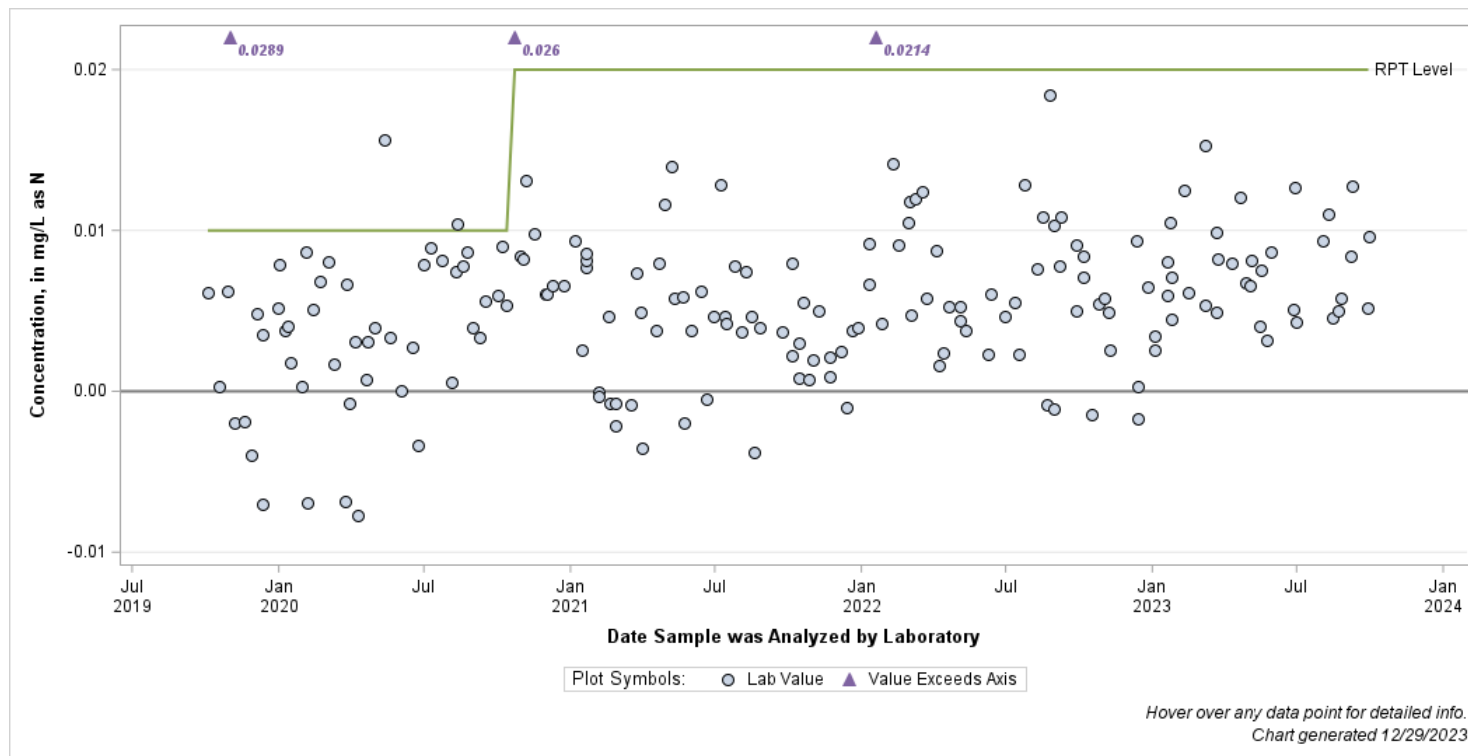


False Positive Rate for Ammonia (NH₃ + NH₄⁺; as N), FIL, DA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Ammonia (NH ₃ + NH ₄ ⁺ ; as N), FIL, DA	00608SHC02	2019	1	0	0%
		2020	48	3	6%
		2021	48	1	2%
		2022	48	1	2%
		2023	44	0	0%

**Highlighted if false positive rate > 5%*

Hover over any data point for detailed info.
Chart generated 12/29/2023

**- Ammonia (NH₃ + NH₄⁺; as N), UNF, CFA, Acidified -
Blind Blank Results**
Lab: NWQL, PCode: 00610, MCode: CL017
 Analysis dates: 11/01/19 through 08/04/23
[Open Data Set](#)

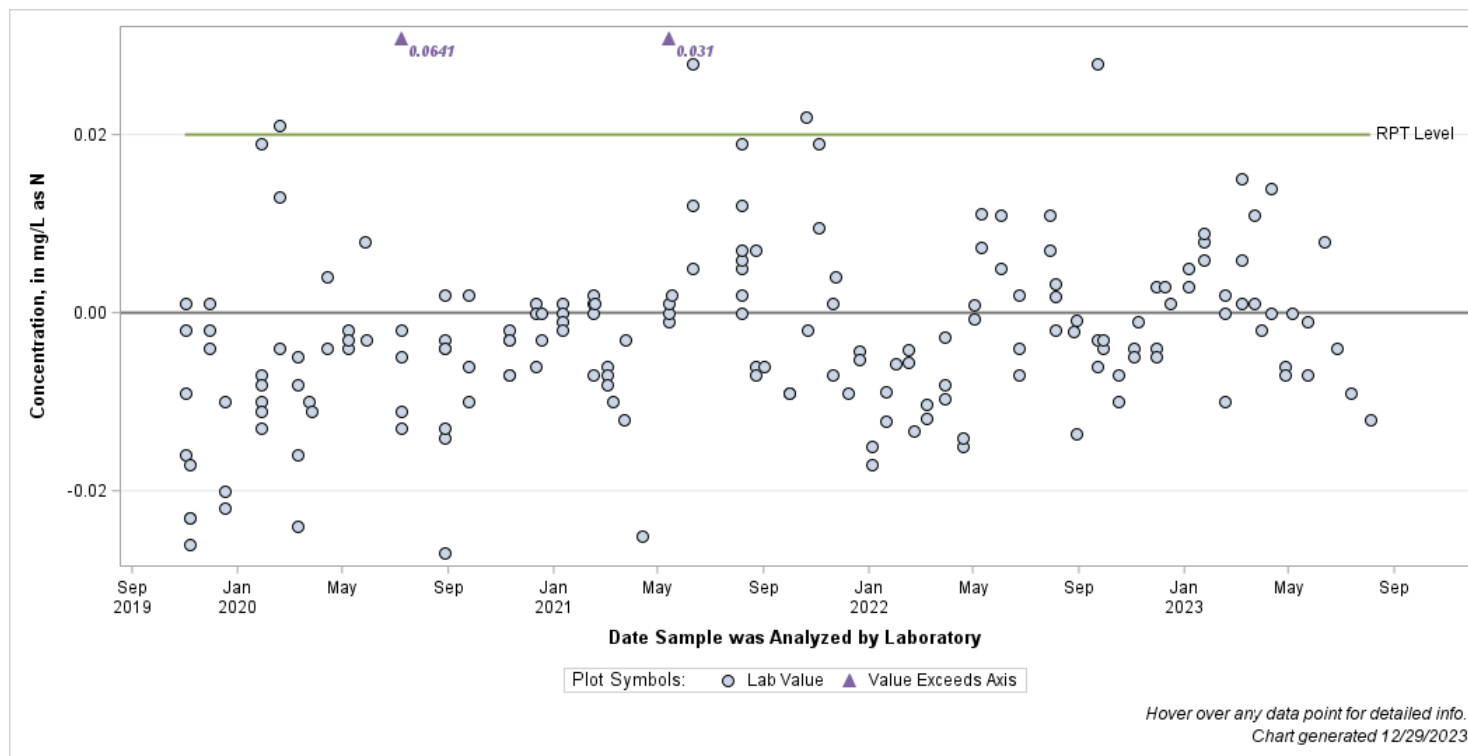

False Positive Rate for Ammonia (NH₃ + NH₄⁺; as N), UNF, CFA, Acidified

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Ammonia (NH ₃ + NH ₄ ⁺ ; as N), UNF, CFA, Acidified	00610CL017	2019	4	0	0%
		2020	48	2	4%
		2021	48	2	4%
		2022	47	2	4%
		2023	35	0	0%

**Highlighted if false positive rate > 5%*

*Hover over any data point for detailed info.
Chart generated 12/29/2023*


- Kjeldahl Nitrogen (NH3+NH4 plus org N; as N), FIL, CFA -

Blind Blank Results

Lab: NWQL, PCode: 00623, MCode: KJ002

Analysis dates: 10/03/19 through 09/18/23

[Open Data Set](#)

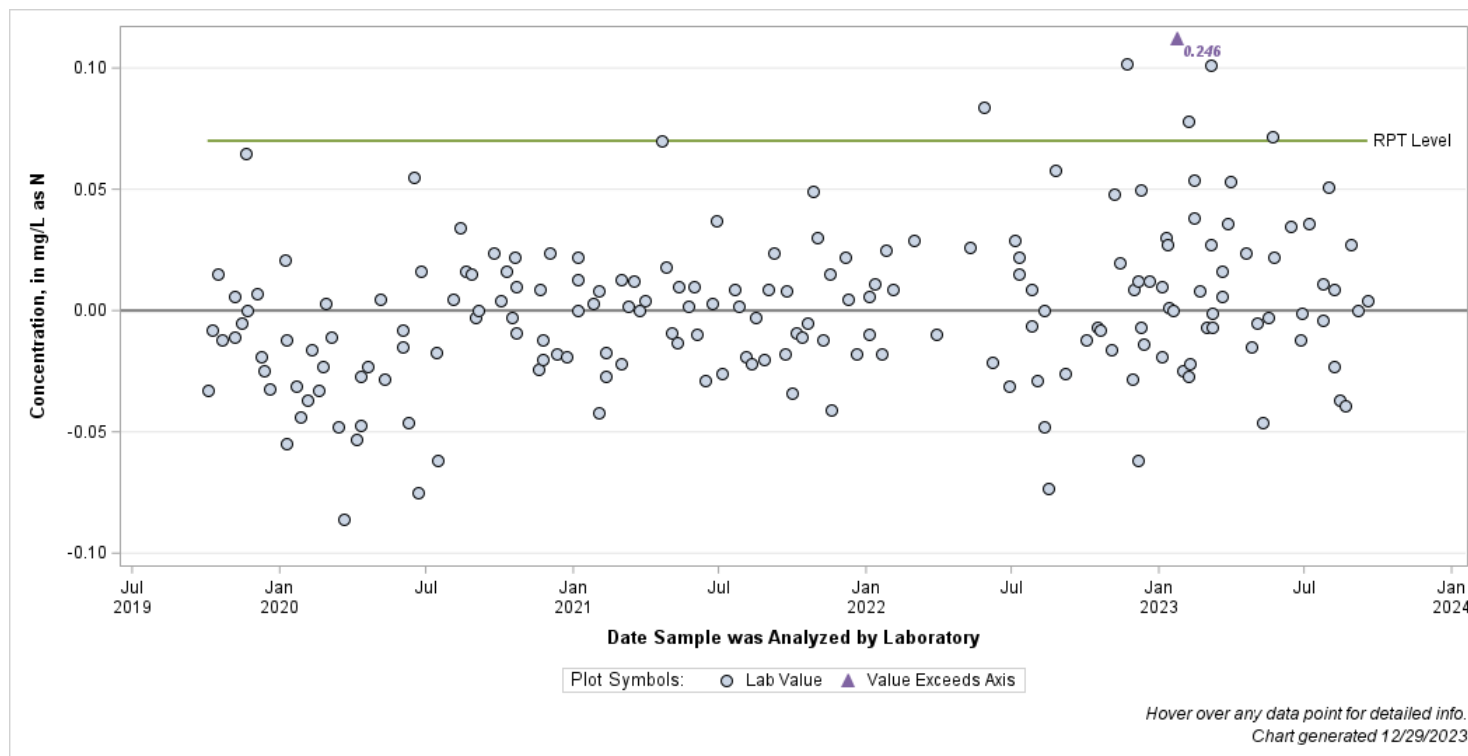

False Positive Rate for Kjeldahl Nitrogen (NH3+NH4 plus org N; as N), FIL, CFA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Kjeldahl Nitrogen (NH3+NH4 plus org N; as N), FIL, CFA	00623KJ002	2019	2	0	0%
		2020	48	0	0%
		2021	48	0	0%
		2022	47	4	9%
		2023	45	2	4%

**Highlighted if false positive rate > 5%*

Hover over any data point for detailed info.
Chart generated 12/29/2023


- Kjeldahl Nitrogen (NH3+NH4 plus org N; as N), UNF, CFA, ACD -

Blind Blank Results

Lab: NWQL, PCode: 00625, MCode: KJ008

Analysis dates: 10/02/19 through 08/04/23

[Open Data Set](#)

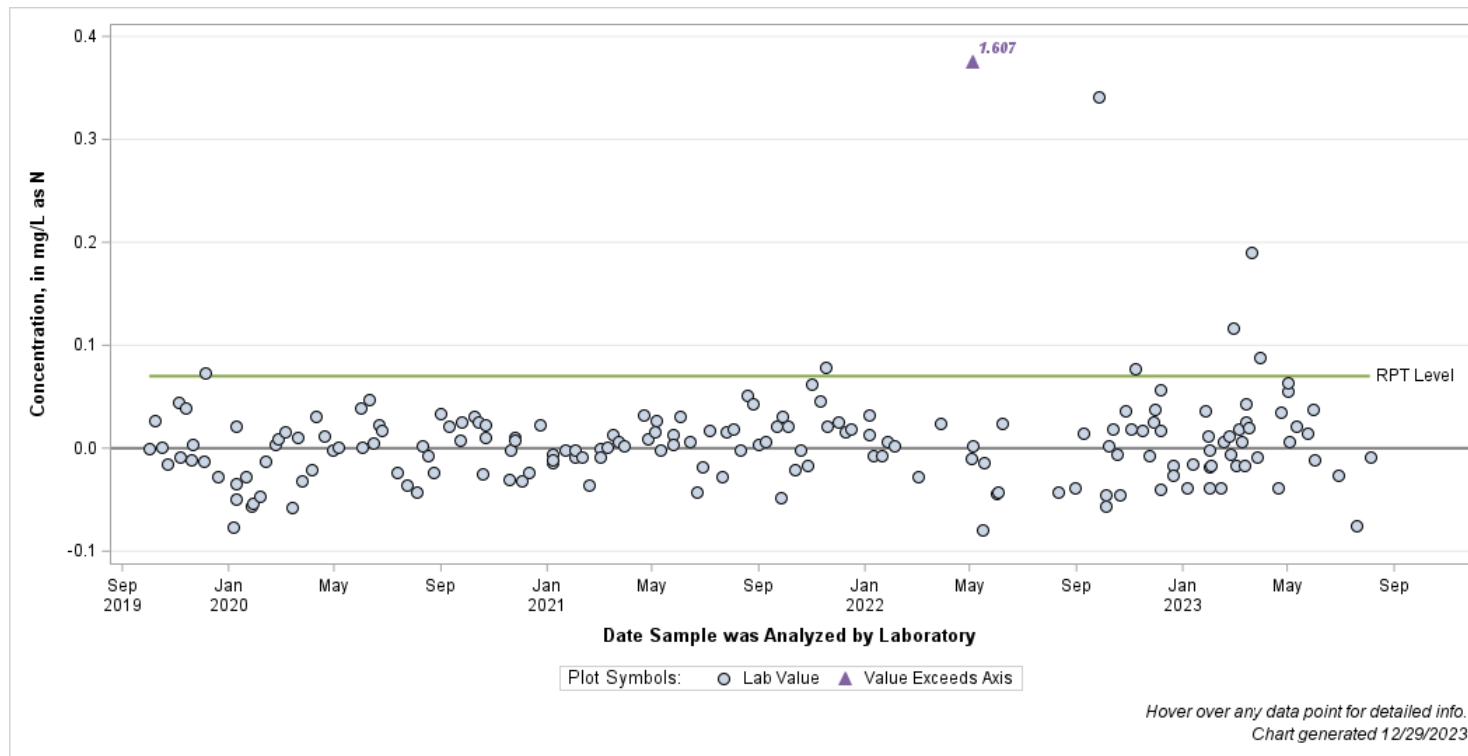


False Positive Rate for Kjeldahl Nitrogen (NH3+NH4 plus org N; as N), UNF, CFA, ACD

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Kjeldahl Nitrogen (NH3+NH4 plus org N; as N), UNF, CFA, ACD	00625KJ008	2019	2	0	0%
		2020	48	1	2%
		2021	48	0	0%
		2022	48	4	8%
		2023	35	3	9%

*Highlighted if false positive rate > 5 %

Hover over any data point for detailed info.
Chart generated 12/29/2023

- Nitrate plus Nitrite (as N), FIL, DA -
Blind Blank Results
Lab: NWQL, PCode: 00631, MCode: RED01
 Analysis dates: 10/02/19 through 09/29/23
[Open Data Set](#)

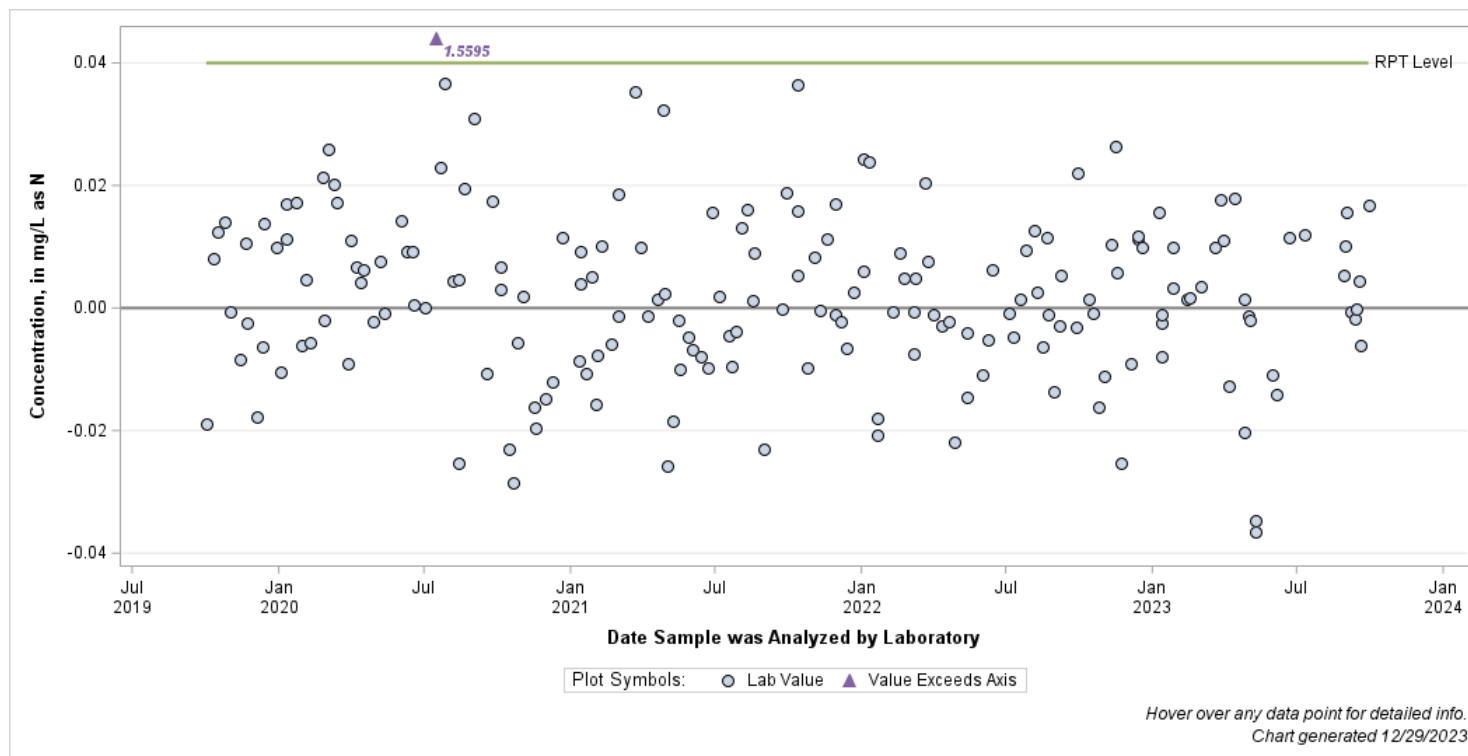


False Positive Rate for Nitrate plus Nitrite (as N), FIL, DA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Nitrate plus Nitrite (as N), FIL, DA	00631RED01	2019	1	0	0%
		2020	48	1	2%
		2021	48	0	0%
		2022	48	0	0%
		2023	43	0	0%

*Highlighted if false positive rate > 5 %

Hover over any data point for detailed info.
Chart generated 12/29/2023

- Nitrate plus Nitrite (as N), FIL, DA, LL -
Blind Blank Results
Lab: NWQL, PCode: 00631, MCode: RED02
 Analysis dates: 10/09/19 through 09/28/23
[Open Data Set](#)

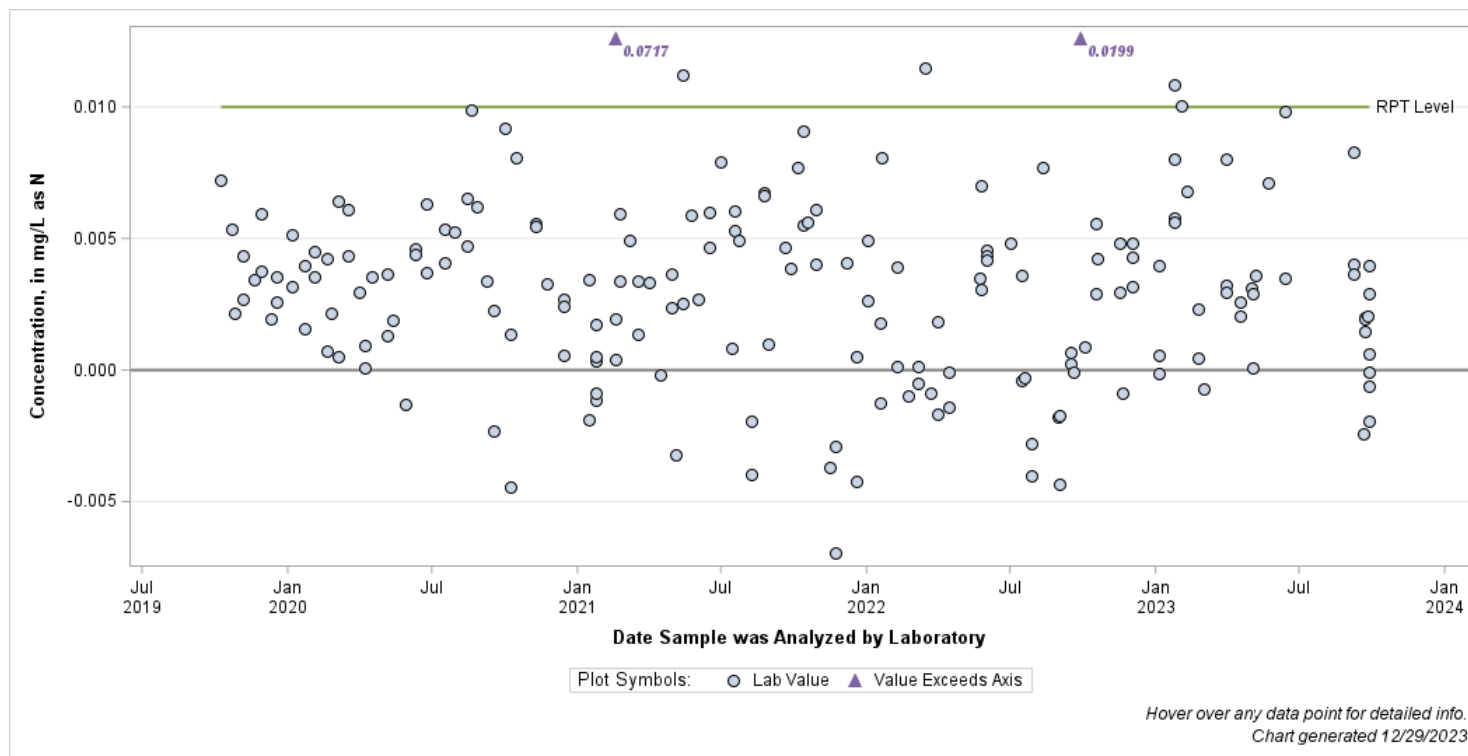


False Positive Rate for Nitrate plus Nitrite (as N), FIL, DA, LL

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Nitrate plus Nitrite (as N), FIL, DA, LL	00631RED02	2020	48	0	0%
		2021	48	2	4%
		2022	48	2	4%
		2023	46	2	4%

*Highlighted if false positive rate > 5%

Hover over any data point for detailed info.
Chart generated 12/29/2023

- Nitrite (as N), FIL, DA -
Blind Blank Results
Lab: NWQL, PCode: 00613, MCode: DZ001
 Analysis dates: 10/04/19 through 09/29/23
[Open Data Set](#)

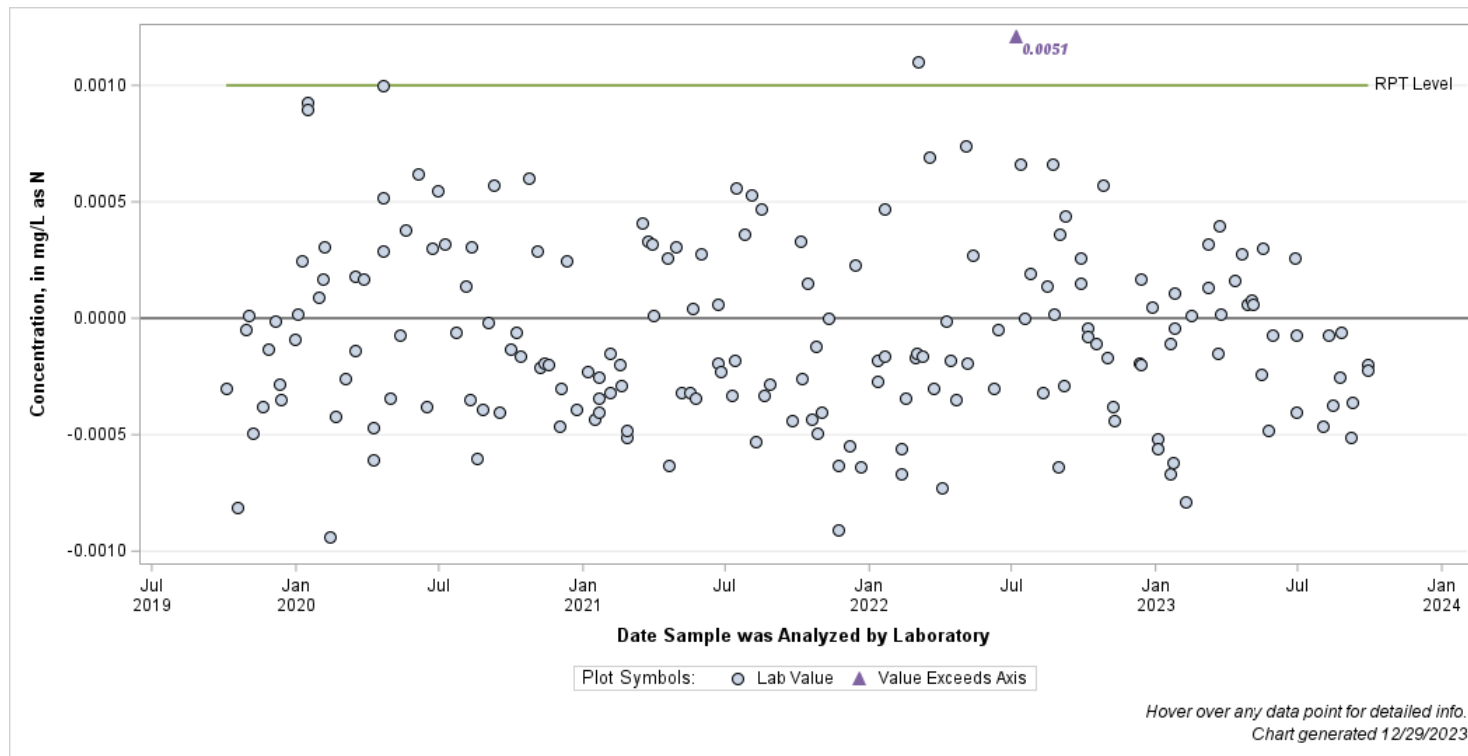


False Positive Rate for Nitrite (as N), FIL, DA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Nitrite (as N), FIL, DA	00613DZ001	2019	1	0	0%
		2020	48	0	0%
		2021	48	0	0%
		2022	48	2	4%
		2023	44	0	0%

**Highlighted if false positive rate > 5 %*

*Hover over any data point for detailed info.
Chart generated 12/29/2023*

- Orthophosphate (as P), FIL, DA -
Blind Blank Results
Lab: NWQL, PCode: 00671, MCode: PHM01
 Analysis dates: 10/04/19 through 09/29/23
[Open Data Set](#)

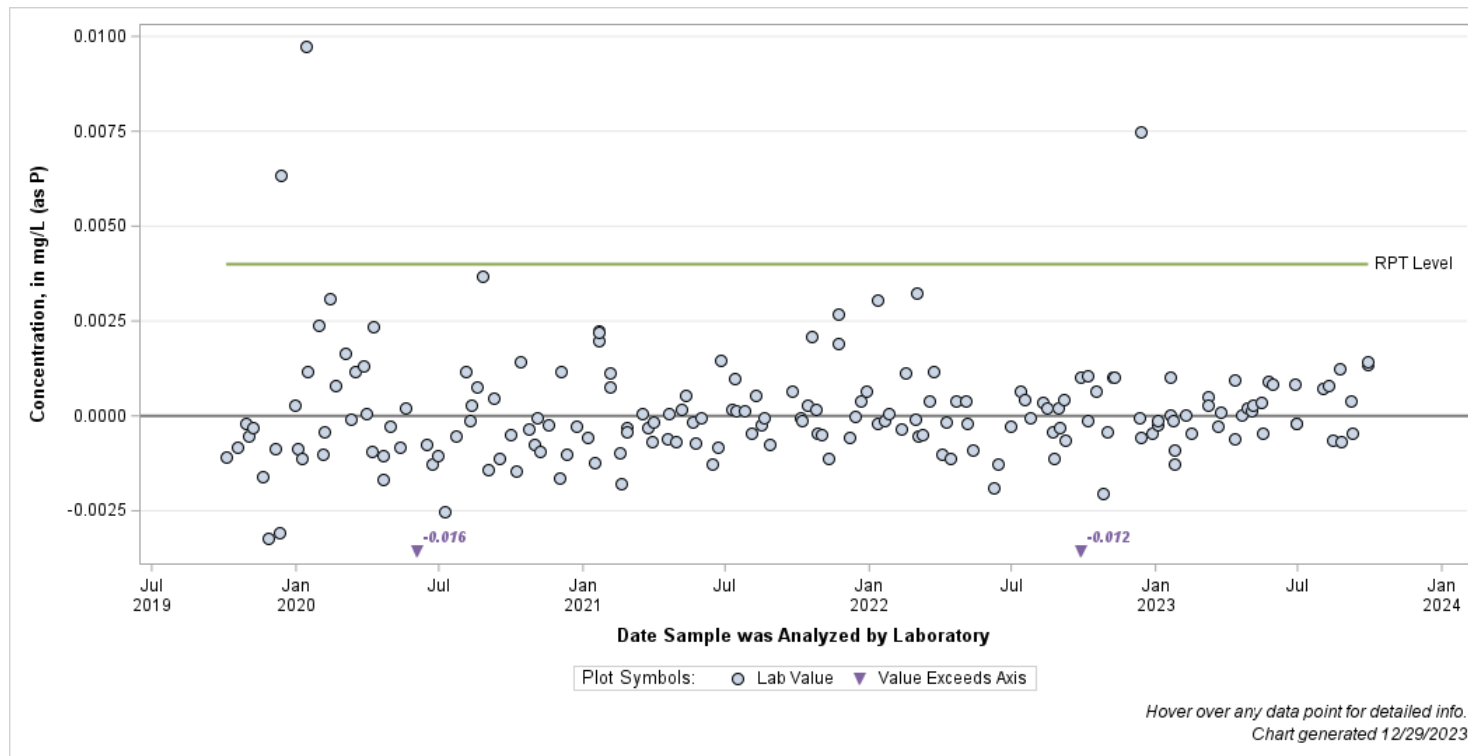


False Positive Rate for Orthophosphate (as P), FIL, DA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Orthophosphate (as P), FIL, DA	00671PHM01	2019	1	0	0%
		2020	48	2	4%
		2021	48	0	0%
		2022	48	0	0%
		2023	44	1	2%

*Highlighted if false positive rate > 5%

Hover over any data point for detailed info.
Chart generated 12/29/2023

- Phosphorus (as P), UNF, ASF, Kjeldahl -
Blind Blank Results
Lab: NWQL, PCode: 00665, MCode: KJ009
 Analysis dates: 10/02/19 through 08/04/23
[Open Data Set](#)

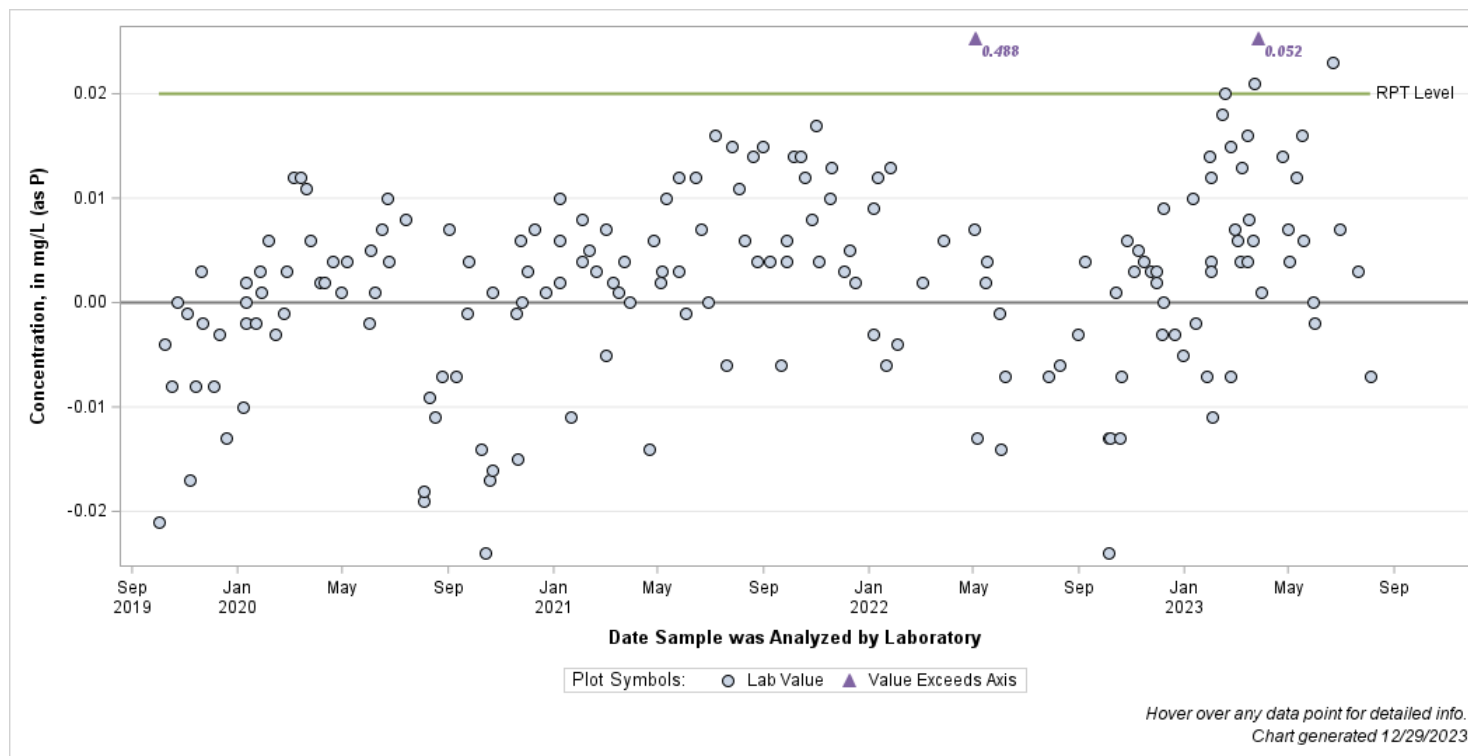

False Positive Rate for Phosphorus (as P), UNF, ASF, Kjeldahl

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus (as P), UNF, ASF, Kjeldahl	00665KJ009	2019	2	0	0%
		2020	48	0	0%
		2021	48	0	0%
		2022	48	1	2%
		2023	35	3	9%

**Highlighted if false positive rate > 5 %*

*Hover over any data point for detailed info.
Chart generated 12/29/2023*


- Phosphorus (as P), UNF, CFA, ACD-P, LL -

Blind Blank Results

Lab: NWQL, PCode: 00665, MCode: CL021

Analysis dates: 10/01/19 through 08/22/23

[Open Data Set](#)

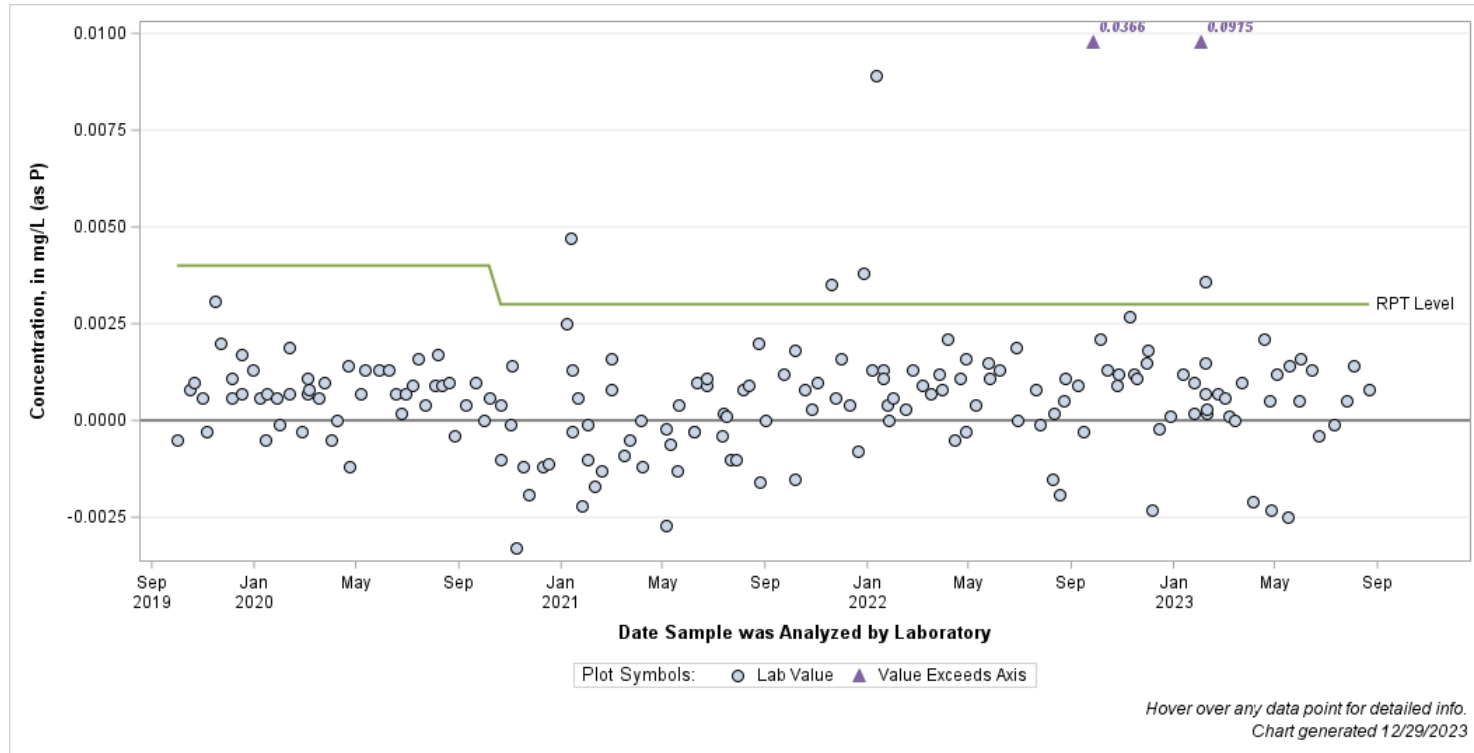


False Positive Rate for Phosphorus (as P), UNF, CFA, ACD-P, LL

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus (as P), UNF, CFA, ACD-P, LL	00665CL021	2019	1	0	0%
		2020	48	0	0%
		2021	48	1	2%
		2022	48	4	8%
		2023	35	2	6%

*Highlighted if false positive rate > 5%

Hover over any data point for detailed info.
Chart generated 12/29/2023

**- Phosphorus (as P), UNF, CFA, ALK-P, ACD -
Blind Blank Results**
Lab: NWQL, PCode: 00665, MCode: AKP01
 Analysis dates: 10/02/19 through 08/29/23
[Open Data Set](#)

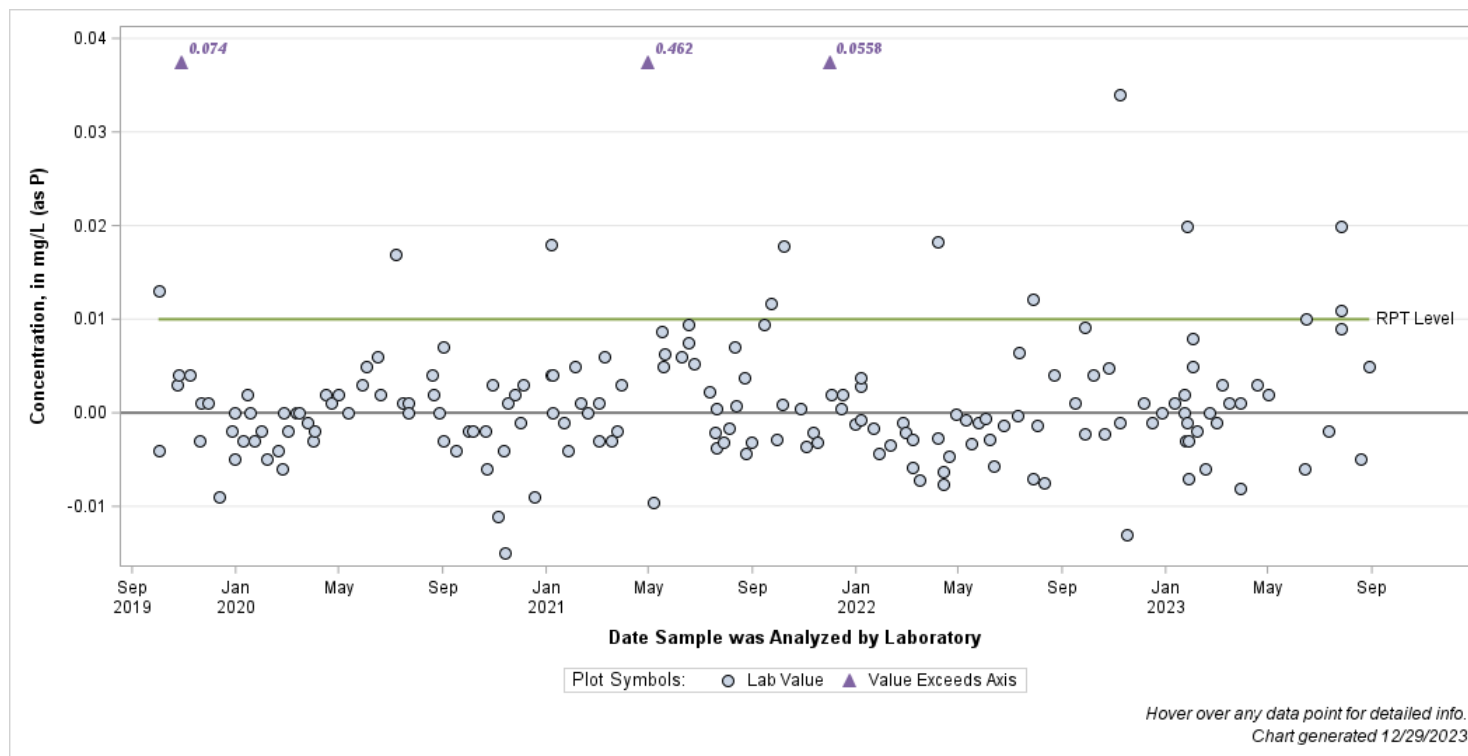


False Positive Rate for Phosphorus (as P), UNF, CFA, ALK-P, ACD

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus (as P), UNF, CFA, ALK-P, ACD	00665AKP01	2019	2	1	50%
		2020	48	2	4%
		2021	48	3	6%
		2022	48	5	10%
		2023	33	3	9%

**Highlighted if false positive rate > 5 %*

*Hover over any data point for detailed info.
Chart generated 12/29/2023*

- Phosphorus as P, FIL, ASF, Kjeldahl -
Blind Blank Results
Lab: NWQL, PCode: 00666, MCode: KJ005
 Analysis dates: 10/03/19 through 09/18/23
[Open Data Set](#)

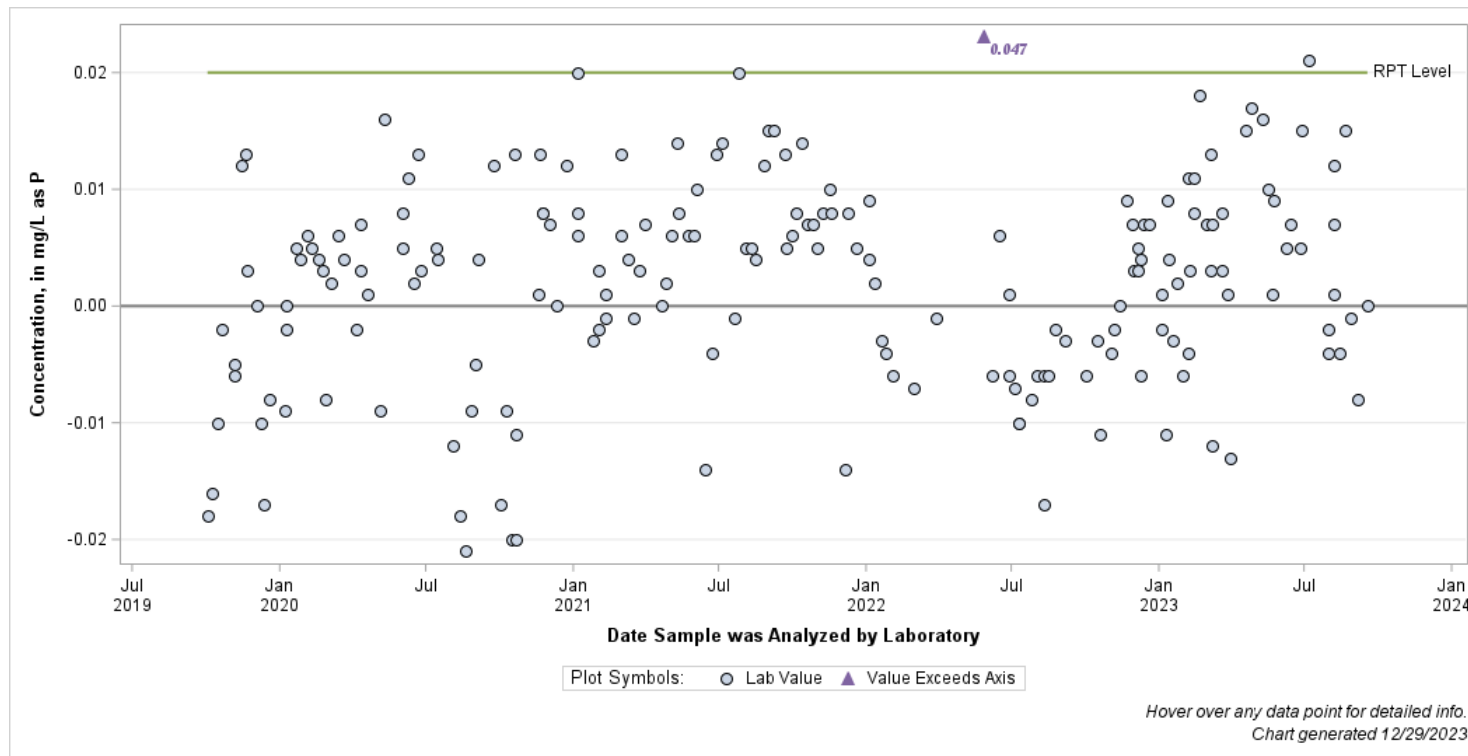


False Positive Rate for Phosphorus as P, FIL, ASF, Kjeldahl

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus as P, FIL, ASF, Kjeldahl	00666KJ005	2019	2	0	0%
		2020	48	0	0%
		2021	48	0	0%
		2022	47	1	2%
		2023	45	1	2%

*Highlighted if false positive rate > 5%

Hover over any data point for detailed info.
Chart generated 12/29/2023

- Phosphorus as P, FIL, CFA, ACD-P, LL -
Blind Blank Results
Lab: NWQL, PCode: 00666, MCode: CL020
 Analysis dates: 10/01/19 through 09/28/23
[Open Data Set](#)

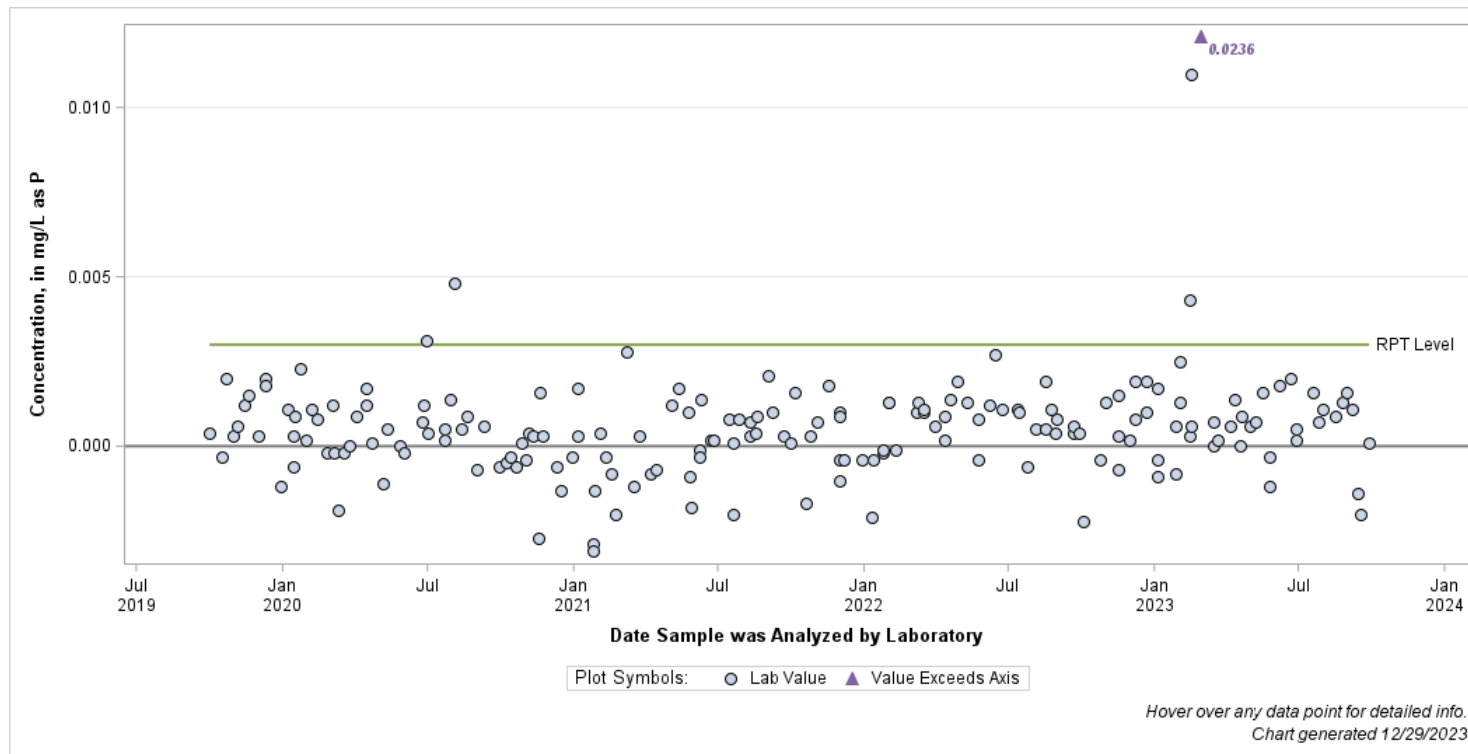

False Positive Rate for Phosphorus as P, FIL, CFA, ACD-P, LL

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus as P, FIL, CFA, ACD-P, LL	00666CL020	2019	1	0	0%
		2020	48	2	4%
		2021	48	0	0%
		2022	48	0	0%
		2023	44	3	7%

**Highlighted if false positive rate > 5 %*

*Hover over any data point for detailed info.
Chart generated 12/29/2023*


- Phosphorus as P, FIL, CFA, ALK-P -

Blind Blank Results

Lab: NWQL, PCode: 00666, MCode: CL063

Analysis dates: 10/09/19 through 09/01/23

[Open Data Set](#)

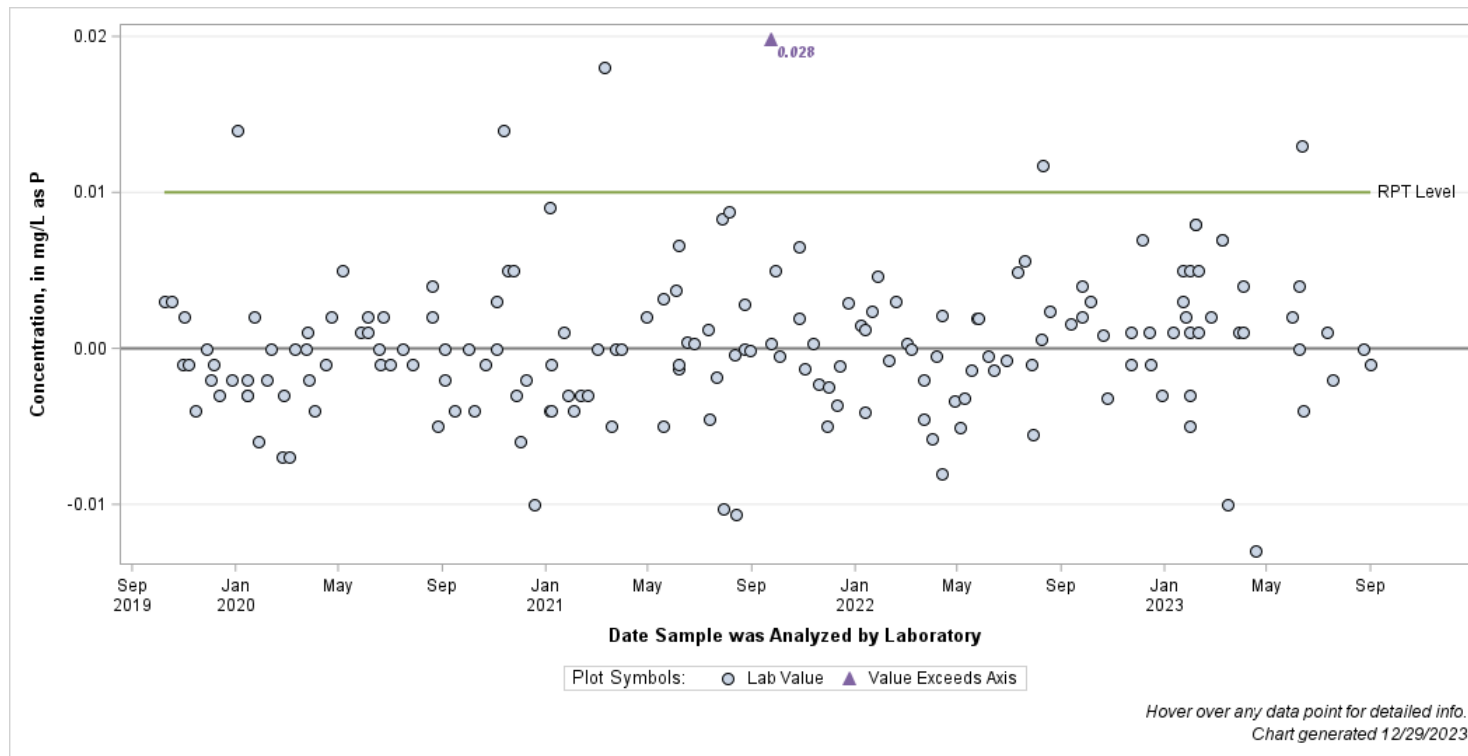

False Positive Rate for Phosphorus as P, FIL, CFA, ALK-P

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus as P, FIL, CFA, ALK-P	00666CL063	2019	1	0	0%
		2020	47	1	2%
		2021	47	3	6%
		2022	48	1	2%
		2023	34	1	3%

*Highlighted if false positive rate > 5%

Hover over any data point for detailed info.
Chart generated 12/29/2023


- Total Nitrogen (NH3+NO3+NO2 plus org N), FIL, CFA, ALK-P -

Blind Blank Results

Lab: NWQL, PCode: 62854, MCode: CL063

Analysis dates: 10/09/19 through 09/01/23

[Open Data Set](#)

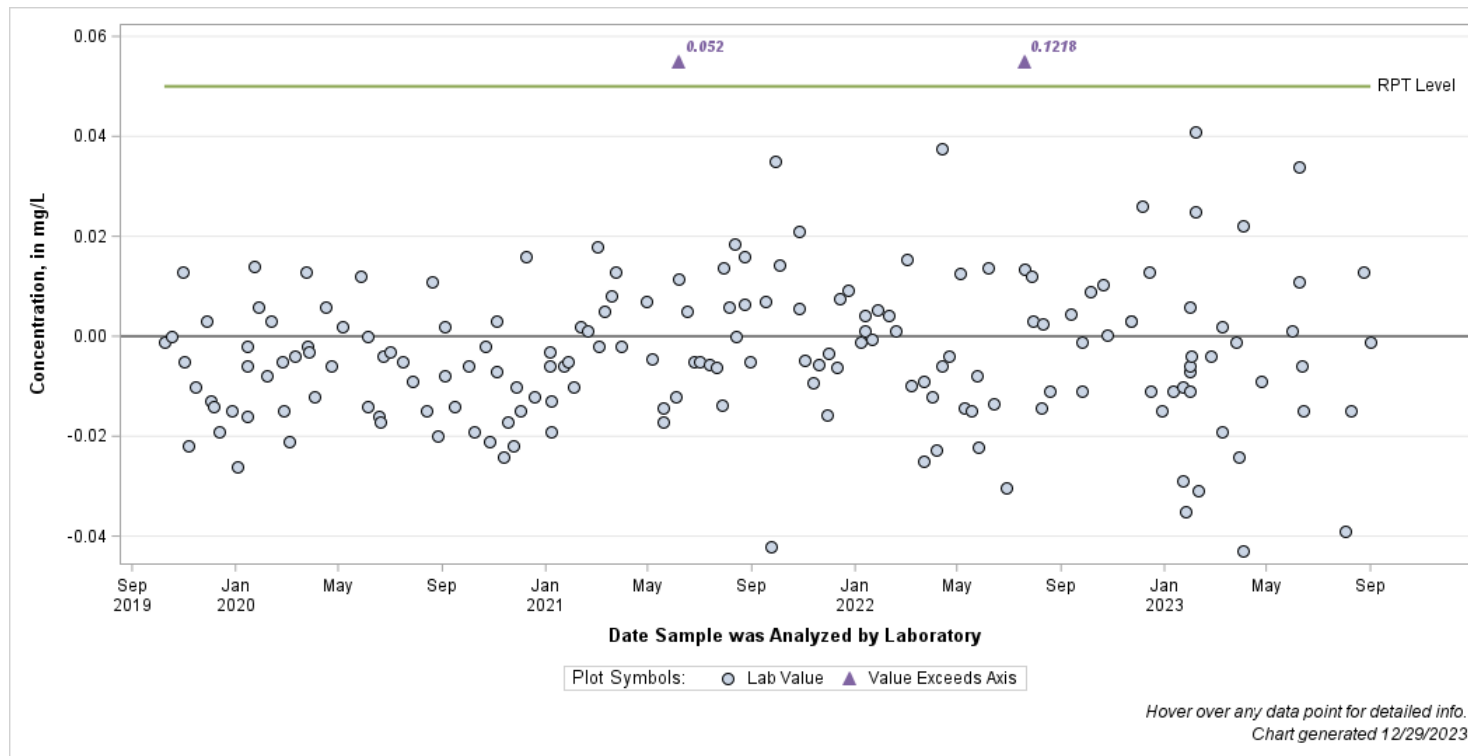

False Positive Rate for Total Nitrogen (NH3+NO3+NO2 plus org N), FIL, CFA, ALK-P

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Total Nitrogen (NH3+NO3+NO2 plus org N), FIL, CFA, ALK-P	62854CL063	2019	1	0	0%
		2020	48	0	0%
		2021	48	1	2%
		2022	48	1	2%
		2023	34	0	0%

*Highlighted if false positive rate > 5%

Hover over any data point for detailed info.
Chart generated 12/29/2023


- Total Nitrogen (NH3+NO3+NO2+org N), UNF, CFA, ALK-P, ACD -

Blind Blank Results

Lab: NWQL, PCode: 62855, MCode: AKP01

Analysis dates: 10/02/19 through 08/29/23

[Open Data Set](#)

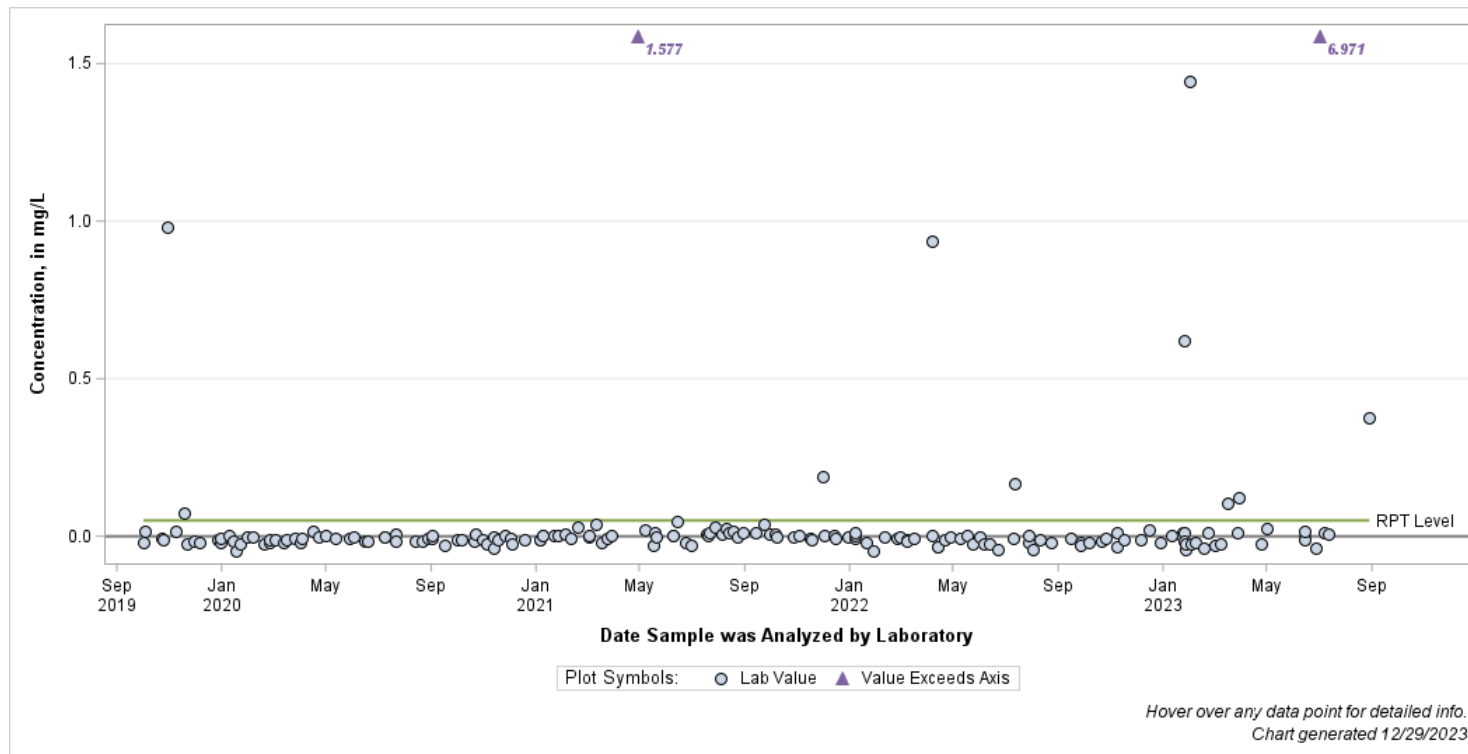

False Positive Rate for Total Nitrogen (NH3+NO3+NO2+org N), UNF, CFA, ALK-P, ACD

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Total Nitrogen (NH3+NO3+NO2+org N), UNF, CFA, ALK-P, ACD	62855AKP01	2019	2	0	0%
		2020	48	2	4%
		2021	48	1	2%
		2022	48	3	6%
		2023	33	6	18%

*Highlighted if false positive rate > 5 %

Hover over any data point for detailed info.
Chart generated 12/29/2023

